

IBR Messtechnik GmbH & Co. KG
Ringstr. 5
D-36166 Haunetal
Fon : +49 6673 900910
Web : www.IBR.com
Email : info@IBR.com


CALIBRATION CERTIFICATE



Type : IMS-5S
Article Number : F350 010
Spring Force : 0.7N
Serial Number : 01176525

Date : 04/28/2025
Testing Device : MFP30 (ID=288967)
Temperature : 20 °C +/-1 °C
Calibration Certificate : 006038 (D-K-15131-01-00)
Measurement Uncertainty : $U = 0,15\mu\text{m} + 2 \times 10^{-6} \times L$

		Tolerance Range [μm]	Deviation [μm]	Exceeding of Tolerance [μm]
Maximum error	fe	2,0	0,3	-
Hysteresis	fu	0,4	0,3	-
Total maximum error	fges	2,0	0,4	-

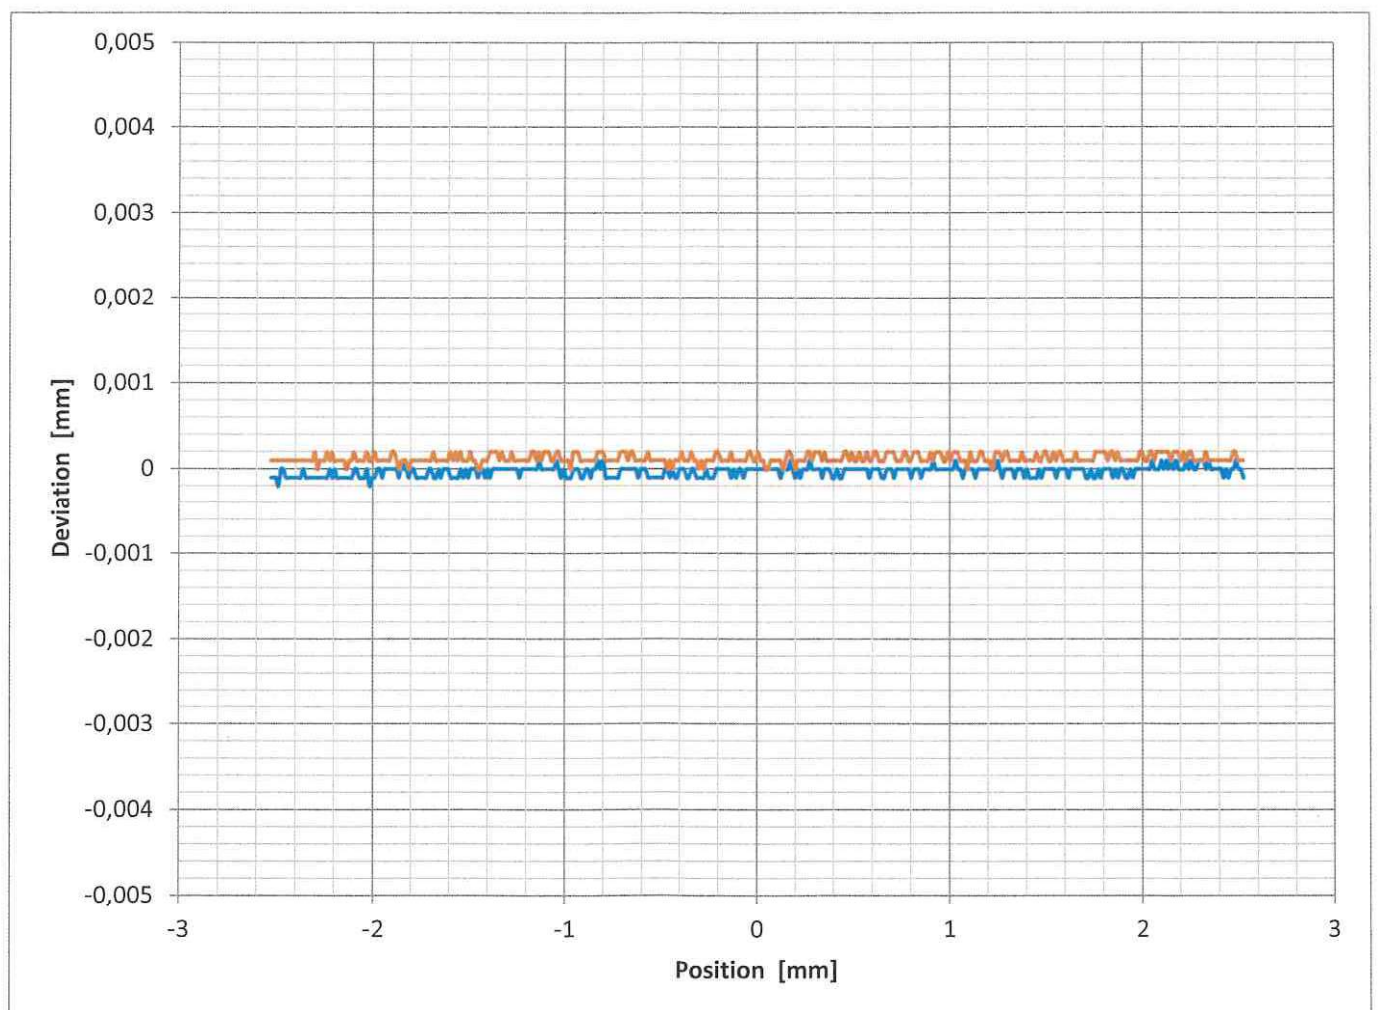

Operator : Michail Omelchenko

Signature :